

## Control the Arterial Mean Blood Pressure in Patient Monitoring System by Predictive Regulator

Nirmalya Chandra<sup>1,a\*</sup> and Dr. Achintya Das<sup>2,b</sup>

<sup>1</sup>Ph.D Scholar, Department of Electronics and Communication Engineering  
Maulana Abul Kalam Azad University of Technology, Haringhata-741249, India

<sup>2</sup>Professor, Department of Electronics and Communication Engineering,  
Kalyani Government Engineering College, Kalyani, Nadia-741235, India under  
Maulana Abul Kalam Azad University of Technology, Haringhata-741249, India

**Abstract :** Continuity in patient monitoring systems during the anaesthesia of *Arterial Mean Blood Pressure* is the crucial obligation for an anaesthetist. This medic assessing system is delusional due to the effect of various types of external and internal parameters. The evaluation of the assessment of *Arterial Mean Blood* pressure is trustworthy anaesthesia for an anaesthetist. The stability of the blood pressure of a patient body is affected before or after the surgical condition of the patient by the surgical disturbance excitation. In this article, we embedded a new technique applying a predictive regulator before the controller. The exploration of this regulator has reduced the deviation in between the predictive value of the feedback path and the referenced desired input so as to the system outcomes would follow the desired optimized trajectory.

**Key Words:** Arterial Mean Blood Pressure, Gain Controller, Predictive Regulator, Steady State Deviation

### I. Introduction

Assessing of *Arterial* blood pressure in a patient body during the time of surgery is very essential. Naturally the pressure is either uplifted or downshifted the normal value at this time. Not but what there an substitute arrangement is processed through injecting a chemical drug (Sodium Nitropruside) into a patient body to regulate the arterial pressure of blood cells [6, 9], but this arrangement has not any systematic base. This provision shows unpredictable feasibility towards patient's satisfaction. Many external disturbances and other factors affect the regulation of arrangement. Blood Pressure is measured with the level of mercury in millimetres unit. (i.e. mmHg) and the method of perception has the mode of three types, i.e. *Systolic*, *Diastolic* and *Mean*. Apart from the first two ones *Mean* blood pressure is considered as the average blood pressure for a systematic body.

The anaesthetists generally concentrate on this *Mean Arterial* pressure of a patient before and

after the time of Surgery. If somehow the level of this mean blood pressure goes underneath, the internal metabolism process of this patient body is disturbed and the liver, nephron, renal, and other neural body parts get affected. Apart from this during the time of surgery of a patient having *Hypertensive* sickness, it is very difficult to operate the machine manually for an anaesthetist. Practically in that time it is very necessary to concentrate the mind of the operator sharply which is actually a strenuous task for a medical unit. The intention of our work in this paper is to construct *optimal predictive moderator* which regulate the variation of these system parameter at the time of anaesthesia of a patient body. Consequently, the previous troublesome effect of a anaesthetist's mind gets relieved.

## II. Review Of The Researcher

Governing the blood pressure spontaneously, the operating system require compatible controller. J. M. Arnsparger et al established two adaptive method mathematically to regulate the blood pressure [1]. R. Meier et al manipulated a *Proportional Integral* controller to control the mean arterial pressure [2] . Masuazawa and Fukui [3] adapted an *LQ-type Optimal Regulator* and general *Adaptive Controller* to control this arterial pressure on patient body. But the researchers could not dominate the default of the actual assessment of blood pressure due to phase delay of system response. In addition Woodruff [4], manipulated a different controller which is tuned itself automatically. This controller is published as *Smith Controller*. However, this controller does not regulate the disturbance perfectly. Now the agility for controlling the blood pressure as its mean value, the improvement of regulator in the system of anaesthesia is *Regulator*. It predicts the change of anaesthesia report to the display machine in advance.

## III. Optimum Regulator in the form of *Predictive Regulator*

An Optimum Regulator is employed to regulate the parameters of open loop system from the existence parameter. The constraints in this system are not saturated in the aggregate. Contrariwise, the Predictive Regulator is associated with *Processing Parameter* and *Feedback Optimization* model. The *Processing Parameter* predicts the best sample from the future controls and then part of Feedback will be embedded into the first Optimal section of the plant. The Predictive Stratagem filters out the impatience present in the outcomes of this

anaesthesia or any other operating process and the constraints of the structure are overcome. In this manner, the robustness of the total anaesthesia as well as the *Mean Arterial Pressure* on the patient body are achieved.

#### IV. Dynamic Feedback Process associated with undesirable Signal

Idealize the following dynamical plant where the undesirable signal is injected externally before the system plant.

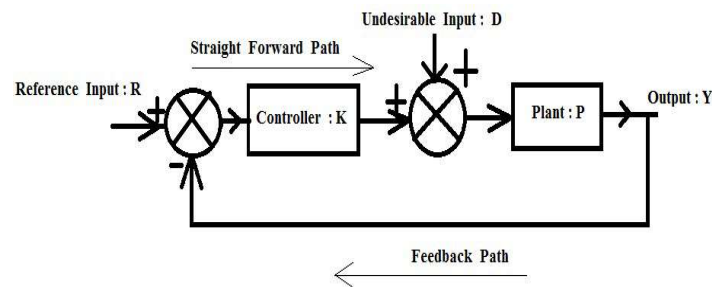


Fig.1. Dynamic feedback process attached with unwanted external input

From the Fig.1, 'R' and 'Y' express the referenced input and outcomes of the system respectively. The undesirable signal 'D' is entered externally into the system. The controller ('K') is connected before the plant 'P'. For straight forward system, the deviation of the system without controller is denoted by,

$$E_s(s) = R(s) - Y(s) = (I - P(s)) \cdot R(s) \quad (1)$$

and with feedback loop for the same system, it is given by,

$$E_f(s) = R(s) \cdot (I + P(s))^{-1} \quad (2)$$

and from Fig.1, the deviation is evaluated as:

$$E = (R - Y) = R - [\{(K \cdot P \cdot R) \cdot (I + K \cdot P)^{-1}\} + \{(P \cdot D) \cdot (I + K \cdot P)^{-1}\}]$$

or,  $E = [\{R - (P \cdot D)\} \cdot \{I + (K \cdot P)\}^{-1}] \quad (3)$

The Eq<sup>n</sup> (3) is pronounced with *Sensitivity* 'S'

$$S = (I + K \cdot P)^{-1} \quad (4)$$

In terms of these, the deviation is given by,

$$E = S \cdot [R - (P \cdot D)] \quad (5)$$

From Eq<sup>n</sup>(4), if '|P \* K|' is large at frequencies, the Sensitivity 'S' have tiny effect.

It signifies the deviation to be less in between the actual outcomes with the desired response. Correspondingly effect of undesired disturbance is also mitigated.

#### V. Assertion of The Controller

In the dynamic plant the controller is uplifted by accompanying the *Predictive Regulator* in a feedback loop system.

In the vicinity of the system defined controller, a predictive mode is applied to bridle the future direction of constraints so as to the outcomes is optimally controlled. The *Performance Objective* collocation is transformed by the squared sum of system parameter. The sum is expressed as the deviation between squared norm of the predicted outcomes and the reference set points of the system and the squared value of the control input in the aspect of future time. This collocation is functioned with the *Weighting (W)* function of *Predictive* and *Control* set point direction  $W_1$  and  $W_2$  respectively as:

$$V(n, N) = W_1 \sum_{n=0}^{N_p} \|y(n, N) - r(N, n)\|^2 + W_2 \sum_{n=0}^{N_c} \|u((n + \Delta N), N) - u(N, n)\|^2 \quad (6)$$

where,  $y(n, N)$  is the predictive outcomes ;  $r(N, n)$  is the reference set point  $u(N, n)$  be the control plant input ;  $N_p$ , and  $N_c$  represents the terminal horizon predictive assumption and the control horizon depends on the sequence number respectively.

The performance of this predictive terminology is conveyed to an operating system as:

- a) Assign the Regulator for advanced movement of input sequence towards future horizon from the instant locus.
- b) Activate the optimum regulator performance initially from the above stated regulation.

**VI. Block Diagram of a Patient Monitoring System**

The following block diagram [5] of Fig.2 is considered as an applied based methodology in our social life :

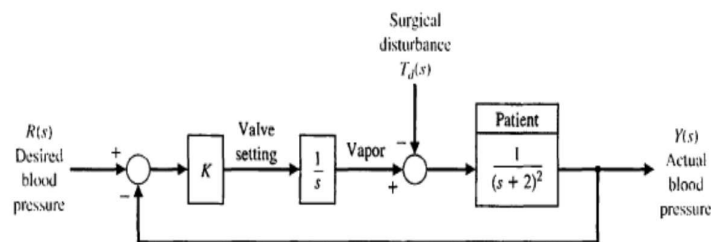


Fig.2. Structure of the medic arrangement to monitor the patient blood pressure

Here, (in the Fig.2) we have considered the patient body system has a 2nd order system. The patient monitoring system gets troubled due to sudden entity of external disturbance. That inconvenience of the anaesthesia affects the total assessing process.

The  $R(s)$  is the intended mean blood pressure.

$Y(s)$  is actual system outcome changed due to undesired disturbance  $T_d(s)$ .

The dissimilation between the set input and the outcomes of measured blood pressure generates omission signal at the steady state condition known as *Steady State Deviation* ( $E(s)$ ).

A controller ( $K$ ) is associated with the horizon of a straight forward system. The Vaporizer acts as this controller here. It constitutes the anaesthesia vapour to the patient.

From the Eq<sup>n</sup> (5) the steady state error is written as:

$$E_s(s) = S * [ R(s) + ((s+2)^{-2} * T_d(s)) ] \quad (7)$$

In the Eq<sup>n</sup> (7) the reference input  $R(s)$  is considered as step input here and the external undesired disturbance excitation is also considered the same characteristic of reference input.

In this manner the error at steady state is expressed as:

$$E_s(s) = \frac{(s^2 + 4s + 5)}{s(s^2 + 4 + 4s) + K} \quad (8)$$

Now the terminal value of this requisite deviation is explained as:

$$e_{ss}(s) = s * E_s(s) = \frac{(s^2 + 4s + 5)}{\left( s^2 + 4s + 4 + \frac{K}{s} \right)} \quad (9)$$

The following Fig.3 shows [7] the characteristic of disturbance input.

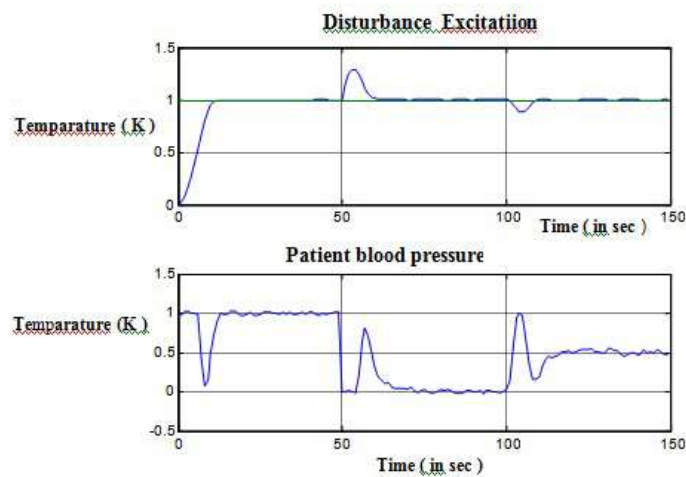


Fig.3. Response of patient blood pressure with disturbance excitation at the monitor

Now reformation of the *Monitoring System* with the *Predictive Regulator* is displayed in the block diagram ( Fig.4).

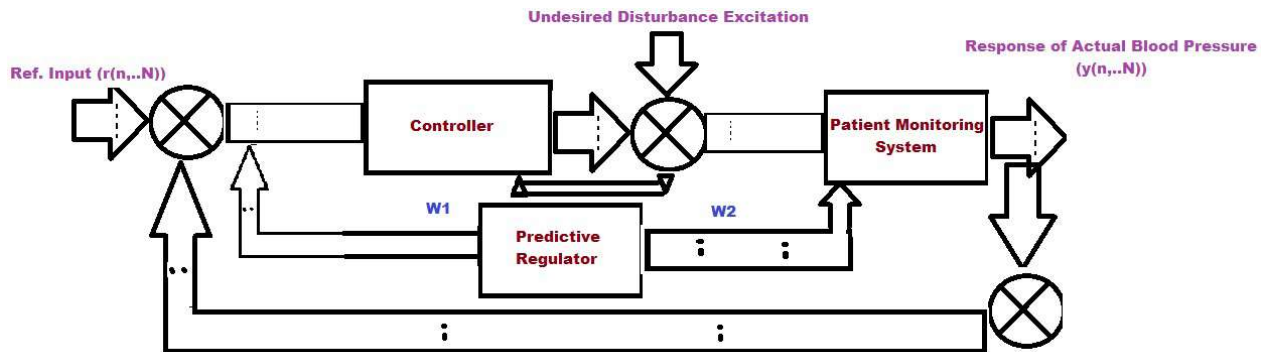


Fig.4. Schematic view of *Blood Pressure Anaesthesia System* using *Predictive Regulator*

The deviations shown in the *Display Oscillator* is regimented by the *Predictive Regulator*. The *Display Oscillator* is connected before the *Patient Monitoring System* in Fig.4. The *steady state deviation* in the operating system is affected due to the change of controller gain connected before the *Vapor* in Fig.2. The controller is reformed by the *Predictive Regulator* in Fig.4 to set the control point of the *Valve*. The corresponding responses of the controller are shown in the *Display Oscillator*.

## VII. Result of the system analysis on the *Display Oscillator*

The *Steady State Deviation* ( Eq<sup>n</sup> (9)) of the Fig.2 is compensated by the *MatLab* simulation of the *Predictive Regulator*. In the following Fig.5, Fig.6 and Fig.7, the characteristic of the *Deviation* in between the Referenced Input and the output from feedback path is plotted. Here we consider the total sample point is 200 and the corresponding dimension of the referenced input is, [1, 3, -1, -2.5, 3.5, 5.4, -4, -6, 5, 2.2]. The dimensions of the referenced input are set by us randomly. The *Predicted Output* from the controller section is try to linked with the *Referenced Input* which is plotted with the *MatLab* simulation in Fig.5, Fig.6, Fig.7 individually. The relation in between '*Np*', and '*Nc*' (*mentioned in section.V*) is set here as-

$$Np = Nc + 10 \quad (10)$$

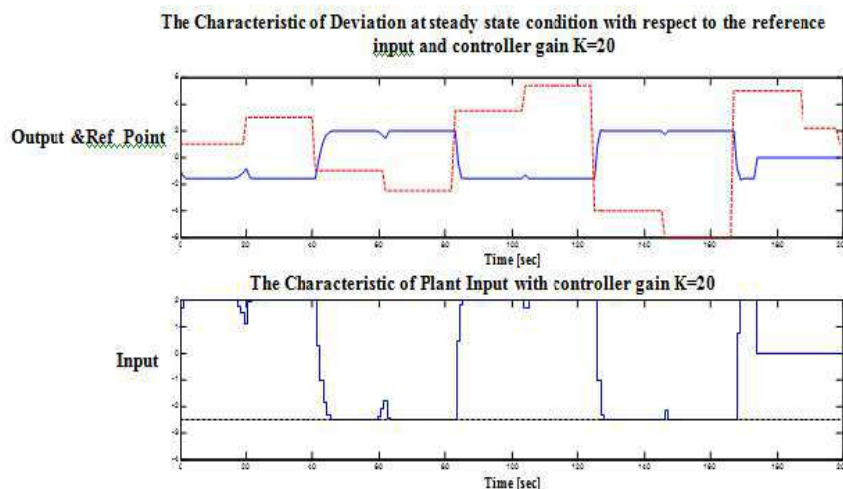


Fig.5. The Characteristic of Deviation at steady state condition with controller gain  $K=20$

In the *Display Oscillator*, the Fig.5 narrates that the deviation in between the *Predictive Output* from the controller section and the Referenced Input is extremely high for the value of  $K$  is 20. The *Controlled Input* is affected due to the presence of disturbance signal.

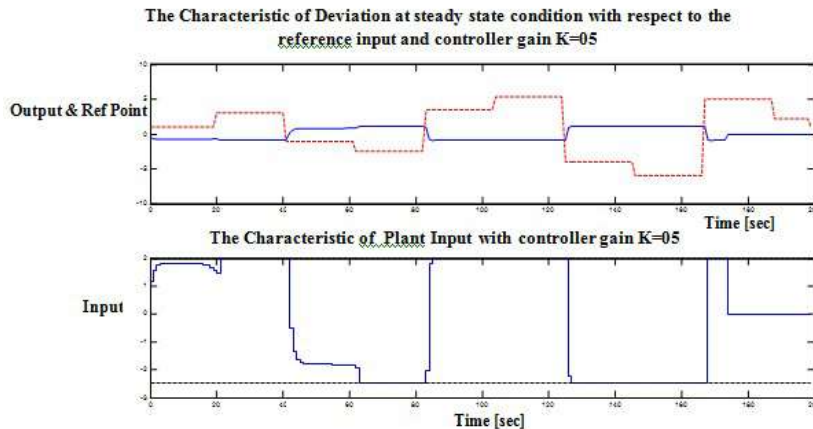


Fig.6. The Characteristic of Deviation at steady state condition with controller gain  $K=05$

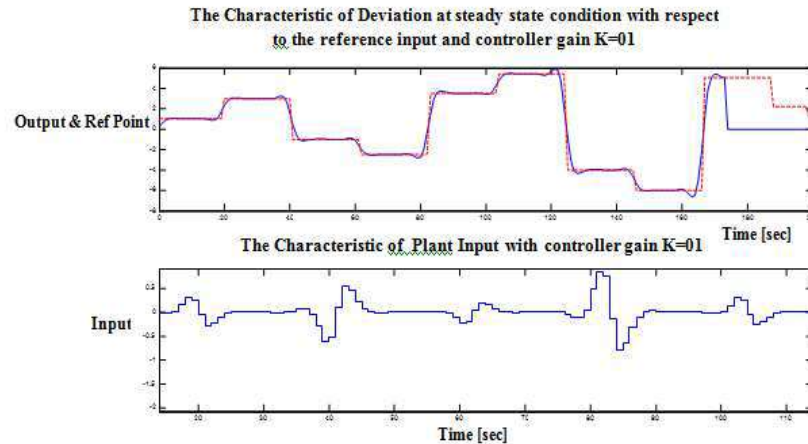


Fig.7. The Characteristic of Deviation at steady state condition with controller gain  $K=01$

In the *Display Oscillator* of the Fig.7, it is displayed that the *Predictive Output* from the controller section emulates the Referenced Input truthfully for the value of  $K$  is 01. The *Controlled Input* is indeed regulated here with the unique value of ' $K$ ' at *Predictive Regulator*. To diminish the deviation in between the output of vapor and the desired reference input at steady state condition the *Predictive Regulator* is designed. The responses of the above figures are for *individual set value* of the controller gain in this medic system. From the above figures shown in the *Display Oscillator*, it is observed that the outcomes of the controller is chasing the trajectory path of desired set input regarding the predictive optimal value taken from the regulator. The deviation is very extensive due to the greater value of the *Valve* ( $K$ ) and the deviation is deficient at the unique value of the *Control Valve* ( $K$ ).

### VIII. Conclusion

The unity controller gain of the *Valve* is the best effort to adjust the predicted value of the outcomes with the referenced input and the analogous controlled input value. When the gain of the controller is increased the lacuna between the output of control section and desired referenced input is grown. It affects the corresponding control input. The response of the controller section is basically the input of the Patient Monitoring System. So to regulation of the *Mean Arterial Blood Pressure* of the monitoring system accurately, we have to regulate the valve setting with the *Predictive Regulator* as per the system requirement.



## References

- [1] J. M. Arnsparger, B. C. McInnis, J. R. Glover, and N. A. Normann, "Adaptive control of blood pressure," *IEEE Trans. on Biomed. Eng.*, vol. BME-30, no. 3, pp. 168-176, 1983
- [2] R. Meier, J. Nieuwland, A.M. Zbinden and S.S. Hacisalihzade, " Fuzzy Logic Control of Blood Pressure during Anesthesia", IEEE Conference on Decision and Control, Arizona, USA, pp. 12-17, December 1992.
- [3] Y. Fukui and T. Masuzawa, "Development of fuzzy blood pressure control system (in Japanese)," *Jpn. J. Med. Electron. Biol. Eng.*, vol. 27. no. 2, pp. 19-25, 1989.
- [4] E. A. Woodruff and R. B. Northrop, "Closed loop regulation of a physiological parameter by an IPFM/SDC (integral pulse frequency modulated/ Smith delay compensator) controller," *IEEE Trans. on Biomed. Eng.*, vol. BME-34, no. 8, pp. 595-602, 1987.
- [5] Richard C. Dorf, Roberth Bishop, "Modern Control System", pp 295 12th Edition PHI Publisher
- [6] Mayo Clinic staff (2009-05-23). "Low blood pressure (hypotension) — Causes". *Mayo Clinic.com. Mayo Foundation for Medical Education and Research*. Retrieved 2010-10-19.
- [7] MATLAB and SIMULINK, The Math Works, Inc, 24 Prime Park Way, Natick, MA 01760.
- [8] Hansen, T. W.; Li, Y.; Boggia, J.; Thijs, L.; Richart, T.; Staessen, J. A. (2010). "Predictive Role of the Nighttime Blood Pressure". *Hypertension* **57** (1):310.doi:10.1161/HYPERTENSIONAHA.109.133900 . ISSN 0194-911X.
- [9] Clark LA, Denby L, Pregibon D, et al. A quantitative analysis of the effects of activity and time of day on the diurnal variations of blood pressure. *Journal of Chronic Diseases*.1987;40:671.
- [10] [Gbenga Ogedegbe](#), MD and [Thomas Pickering](#), MD, DPhil. et al. Principles and techniques of blood pressure measurement. *Cardiol Clin*. Author manuscript; available in PMC 2013 Apr 30. Published in final edited form as: *Cardiol Clin*. 2010 Nov; 28(4): 571–586.doi: [10.1016/j.ccl.2010.07.006](https://doi.org/10.1016/j.ccl.2010.07.006)